

1/3

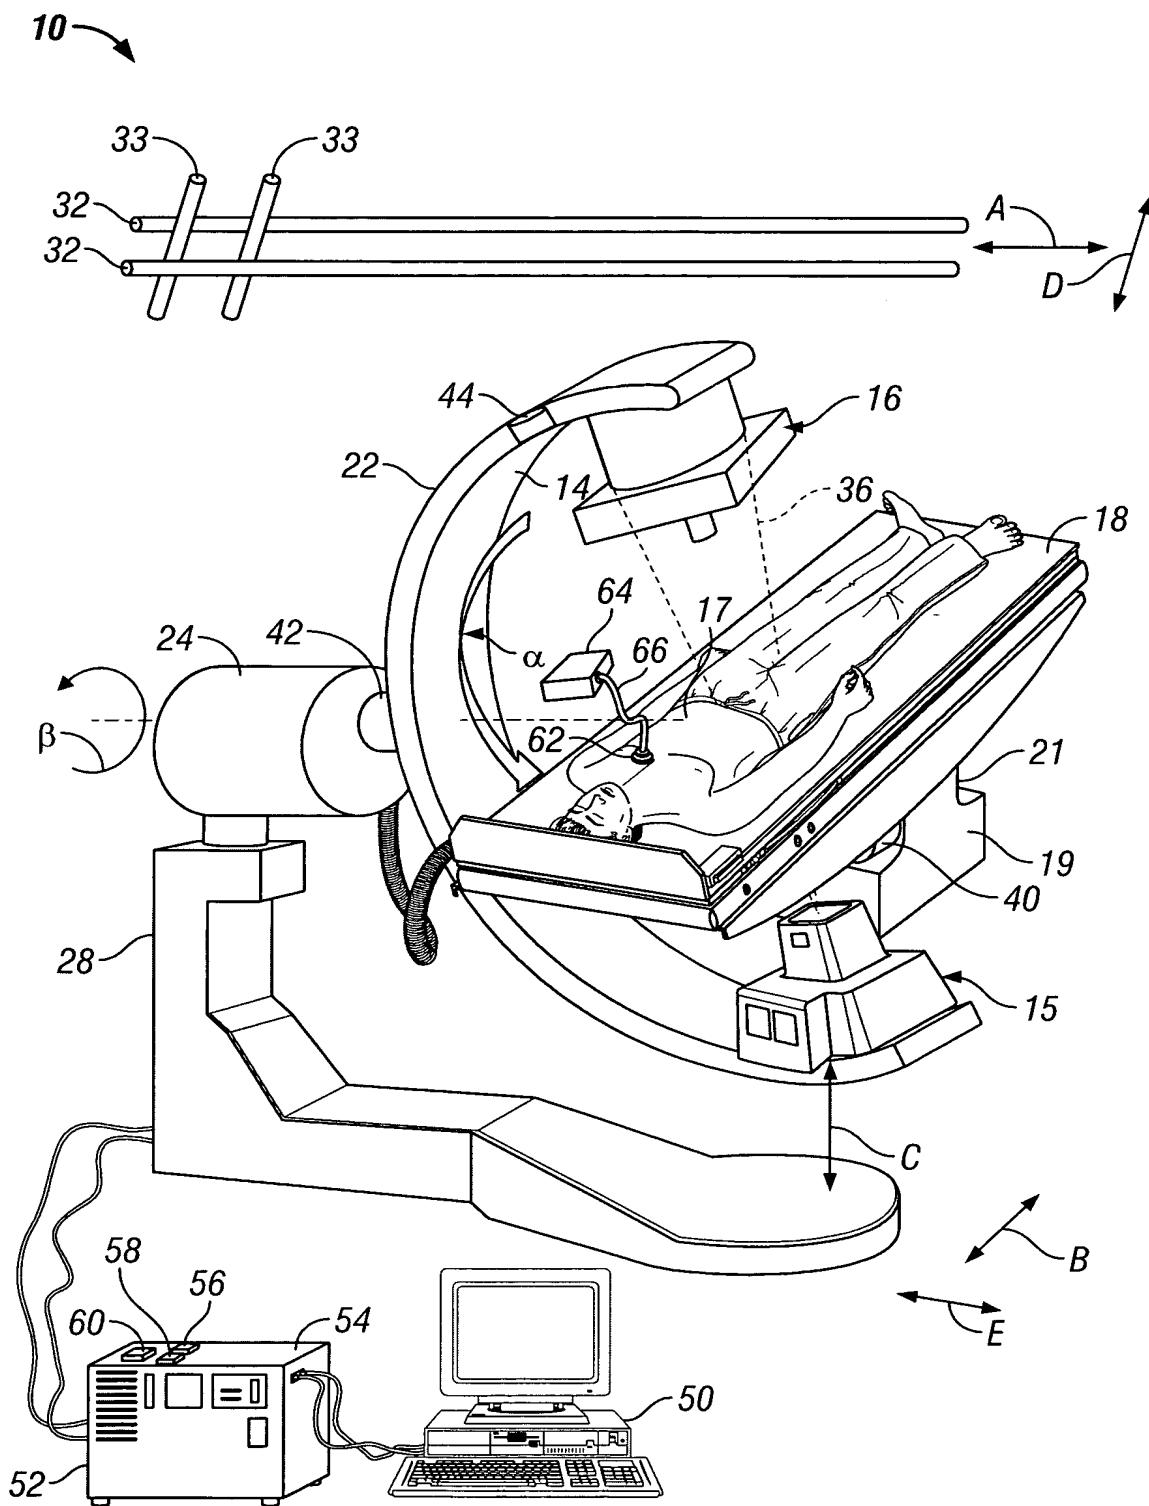


FIG. 1

2/3

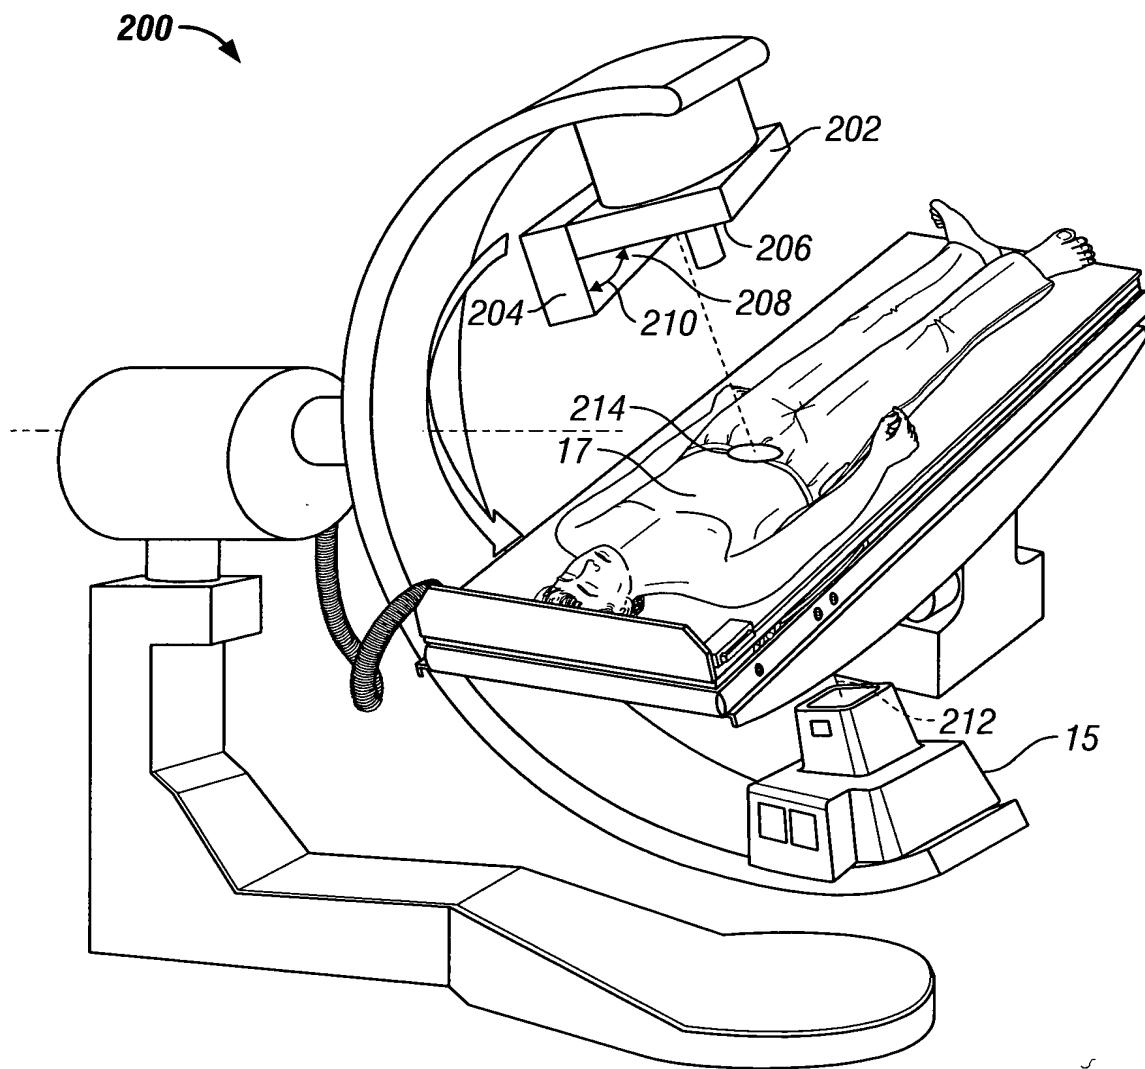


FIG. 2

3/3

300

302

*Aligning a Patient Table in an Opening of an
Opening of a C-ARM Unit that Includes a CZT
Photon Detector Positioned at a First End of
the C-ARM and an X-RAY Source Positioned
at a Second Opposing End of the C-ARM*

304

*Imaging a Patient Utilizing a First Imaging
Modality During a First Portion of a Scan*

306

*Imaging a Patient Utilizing a Second Imaging
Modality During a Second Portion of the Scan*

FIG. 3